128-350.1
G04-9

35

received US PATENT OFFICE Sept 15 1960
(GP335)
D Z Trulucke

DENZ VENTRICULO-ATRIAL SHUNT WITH RTAGH MODIFICATION FLUSHING DEVICE

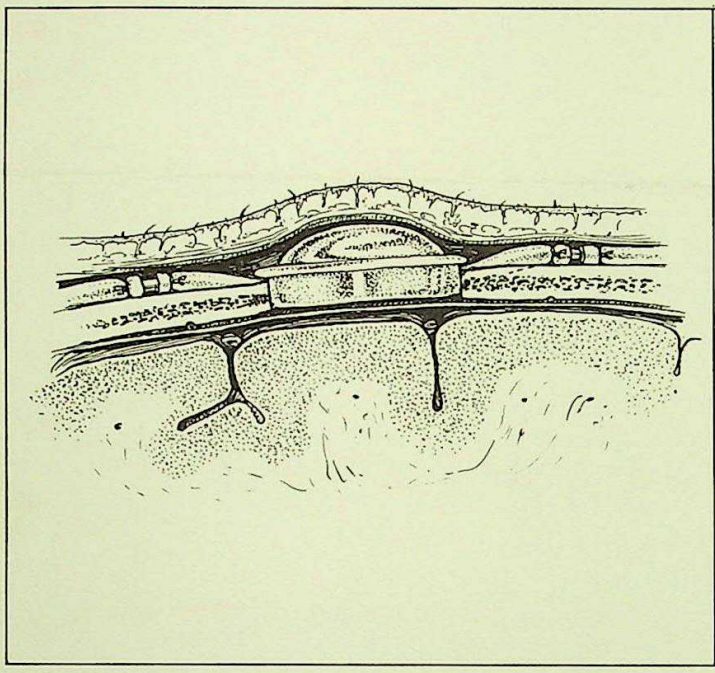

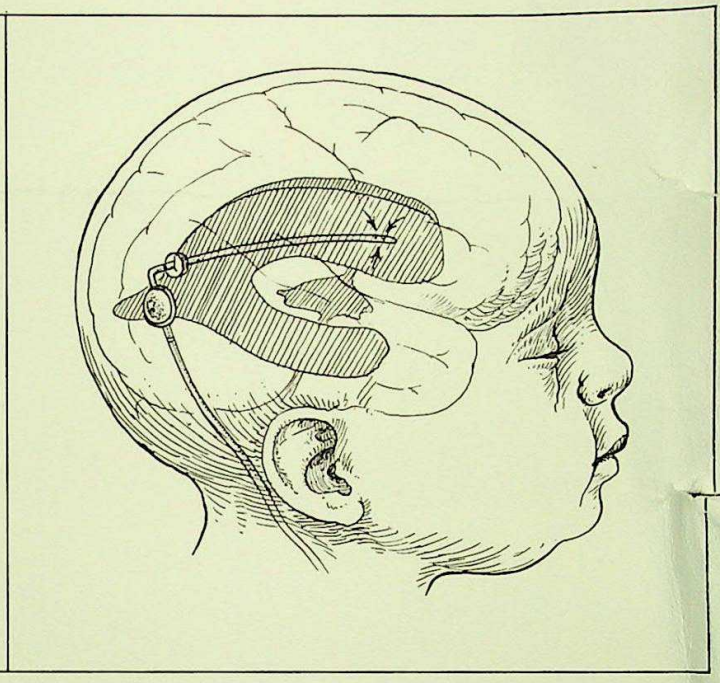

The Murtagh Modification makes it possible for both the inlet and outlet tubes of the Flushing Device to remain outside the skull. The only structure traversing the brain to the ventricle is the pliable ventricular catheter which can be directed into the long axis of the ventricle. If revision is necessary, the pump does not have to be disturbed.

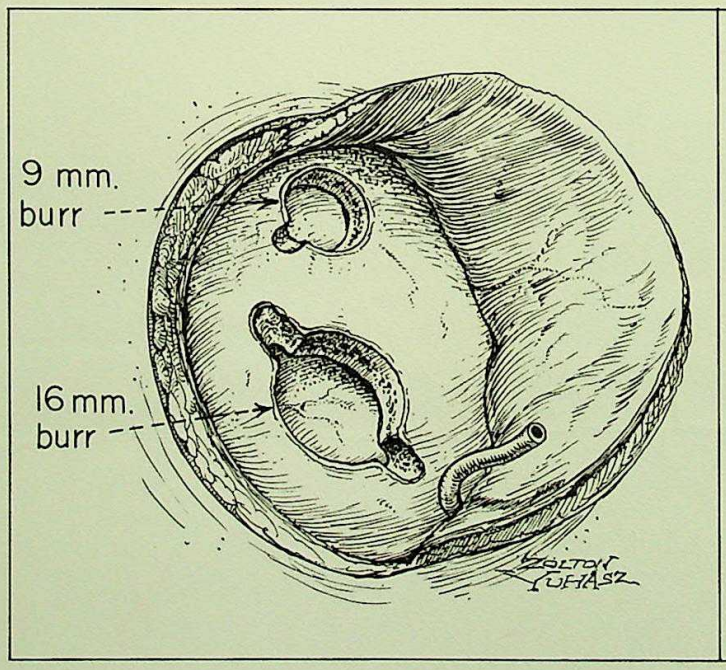

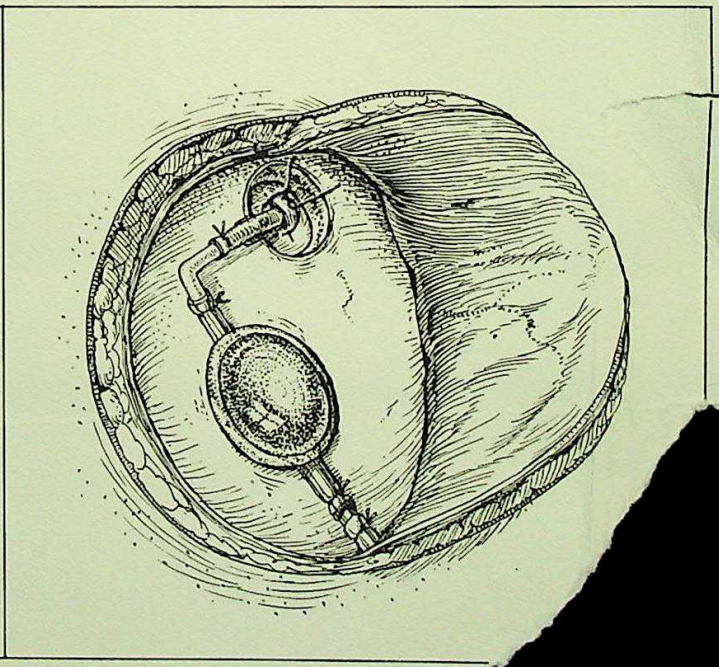

HEYER-SCHULTE CORPORATI

5377 Overpass Road / Santa Barbara / California 93